

Received: 16 June 2011 – Accepted: 7 July 2011 – Published: 14 July 2011

Correspondence to: C. J. Sapart (c.j.sapart@uu.nl)

Published by Copernicus Publications on behalf of the European Geosciences Union.

AMTD

4, 4473–4503, 2011

**Simultaneous stable
isotope analysis of
methane**

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Abstract

Methane and nitrous oxide are important greenhouse gases which show a strong increase in atmospheric mixing ratios since pre-industrial time as well as large variations during past climate changes. The understanding of their biogeochemical cycles can be improved using stable isotope analysis. However, high-precision isotope measurements on air trapped in ice cores are challenging because of the high susceptibility to contamination and fractionation.

Here, we present a dry extraction system for combined CH₄ and N₂O stable isotope analysis from ice core air, using an ice grating device. The system allows simultaneous analysis of $\delta D(CH_4)$ or $\delta^{13}C(CH_4)$, together with $\delta^{15}N(N_2O)$, $\delta^{18}O(N_2O)$ and $\delta^{15}N(NO^+ \text{ fragment})$ on a single ice core sample, using two isotope mass spectrometry systems. The optimum quantity of ice for analysis is about 600g with typical "Holocene" mixing ratios for CH₄ and N₂O. In this case, the reproducibility (1σ) is 2.1 ‰ for $\delta D(CH_4)$, 0.18 ‰ for $\delta^{13}C(CH_4)$, 0.51 ‰ for $\delta^{15}N(N_2O)$, 0.69 ‰ for $\delta^{18}O(N_2O)$ and 1.12 ‰ for $\delta^{15}N(NO^+ \text{ fragment})$. For smaller amounts of ice the standard deviation increases, particularly for N₂O isotopologues. For both gases, small-scale intercalibrations using air and/or ice samples have been carried out with other institutes that are currently involved in isotope measurements of ice core air. Significant differences are shown between the calibration scales, but those offsets are consistent and can be corrected for.

1 Introduction

The atmospheric mixing ratios of methane (CH₄) and nitrous oxide (N₂O) have increased since pre-industrial time, which has contributed significantly to the increased radiative forcing since 1750 (Forster et al., 2007). Furthermore, for both gases, large variations are observed during past climate changes (Spahni et al., 2005). Numerous studies were performed to understand the atmospheric budget of CH₄ and N₂O in

AMTD

4, 4473–4503, 2011

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



the past and to assess climate feedbacks of the natural sources in the climate system (Lelieveld et al., 1998; Dlugokencky et al., 1998, 2009; Bousquet et al., 2006; Etheridge et al., 1998; MacFarling Meure et al., 2006; Flückiger et al., 2002). Still the causes of variability, in particular of the natural sources, are not well understood.

Isotope measurements can be used as a tool to distinguish contributions from individual sources (Brenninkmeijer et al., 2003) and changes in the sink strength. Measurements from the recent past have been obtained from atmospheric measurement networks (Quay et al., 1999; Miller et al., 2002), from archived air samples (Röckmann and Levin, 2005) and from firn air (Bräunlich et al., 2001; Ishijima et al., 2007). To obtain information on earlier atmospheric conditions, ice core air analyses are required. In that case, isotope measurements are particularly challenging, since only a small amount of air is available and extraction artifacts can bias the analysis. Nevertheless, the advent of continuous-flow isotope ratio mass spectrometry (IRMS) (Merritt et al., 1995), has led to the development of numerous analytical systems that only require small amounts of sample (e.g. Rice et al., 2001; Miller et al., 2002; Röckmann et al., 2003b; Brass and Röckmann, 2010) and subsequent analytical systems for ice core analyses (Bernard et al., 2006; Schaefer et al., 2006; Ferretti et al., 2005; Sowers, 2001, 2006; Sowers et al., 2003; Bock et al., 2010b; Behrens et al., 2008). These developments have resulted in a number of interesting findings in the past years (Fischer et al., 2008; Mischler et al., 2009; Sowers, 2001, 2006, 2010; Sowers et al., 2003; Bernard et al., 2006; Ferretti et al., 2005; Bock et al., 2010a; Schäfer et al., 1998) which have, for example, ruled out a strong contribution of marine clathrate decomposition to paleoatmospheric methane changes as observed in ice core air.

Ice extraction systems can be realized as wet extraction systems (after Robbins et al., 1973; Craig and Chou, 1982), dry extraction systems (after Moor and Stauffer, 1984; Etheridge et al., 1988) and sublimation techniques (Gülük et al., 1997, 1998; Schmitt et al., 2011) each with their particular benefits and limitations. A drawback of most of the analytical systems published to date is that they can only measure one single compound per sample. Since ice air is limited and precious, we designed a

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

system where at least two gases can be measured on one ice air sample, namely one isotope signature of CH₄ (δ D or δ^{13} C) and the complete isotopic composition of N₂O (δ^{15} N(N₂O), δ^{18} O(N₂O) and δ^{15} N(NO⁺fragment)). The new method is suited for ice samples of 200–800 g (for ice with mixing ratios of roughly 220–270 ppb for N₂O and 600–700 ppb for CH₄) corresponding to a minimum of ~14–17 ng of CH₄ and ~15 ng of N₂O for Holocene ice, allowing a high temporal resolution for ice core data.

2 Method

2.1 Experimental set-up

The complete analytical system is schematically shown in Fig. 1. A dry extraction technique is coupled to two continuous-flow IRMS systems for simultaneous isotope analysis of CH₄ and N₂O. These parts will be described in detail in the following sub-sections.

2.1.1 Extraction

The extraction device consists of a 6 L stainless steel (SS) pot equipped with a perforated SS cylinder with sharp edges, the so-called “ice-grater” (Etheridge et al. 1988), where an ice core sample is grated under its own weight by sliding back and forth over the grater. The grater fits precisely between bottom plate and lid of the extraction pot in order to avoid metal-metal collisions, which could lead to CH₄ contamination (Higaki et al., 2006). Moreover, the grater is coated with titanium nitride (TiN, BALINIT®A, Oerlikon Blazers) in order to harden and protect the grating surface. Following the introduction of the ice sample into the grating cylinder, the SS pot is sealed with a copper o-ring (conflat flange of 22 cm of diameter) and fixed in a shaking device inside a freezer at –30 °C. From there, the pot can be evacuated to 10^{–3} mb via the vacuum extraction system to remove laboratory air before grating starts. During the grating

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



process, the shaker oscillates with a frequency up to 3Hz (see below) and with an amplitude of about 6 cm. After 20 min of grating following an optimized protocol (see below), 99 % of an ice core piece of 200–800 g has been ground into flakes of 1 to 2 mm diameter.

After the grating, the SS pot is reconnected to the vacuum extraction system (Fig. 1) and the air liberated from the ice is processed through Trap 1 (T1), which traps H₂O at –80 °C, and Trap 2 (T2), which traps CO₂, N₂O and most higher molecular weight hydrocarbons at –196 °C, to Trap 3 (T3). T3 is filled with ~40 ml of Hayesep D (mesh 80/100, Alltech GmbH, Germany), a molecular adsorbent, cooled to –196 °C in a liquid nitrogen bath. This trap acts as a cryopump adsorbing all the air from the SS pot to T3 in 45 min. After extraction, the N₂O–CO₂ mixture trapped in T2 is flushed at ambient temperature to the N₂O IRMS in a Helium (He) carrier gas. Subsequently, T3 is heated to 60 °C and its content is flushed in He to the CH₄ IRMS. Both flushing units operate independently.

2.1.2 Methane IRMS

The CH₄ IRMS system is a fully automated analytical set-up for $\delta D(CH_4)$ or $\delta^{13}(CH_4)$ analyses (Brass and Röckmann, 2010). This system has been used for various laboratory and atmospheric studies in the past (Vigano et al., 2008, 2009, 2010; Keppler et al., 2006, 2008). For ice core-air measurements, the air trapped in T3 is flushed through a 2 position Valco 6 port valve (V1) (VICI® AG International) to the preconcentration unit (PRECON) at a flow rate of 20 ml min⁻¹. The PRECON of the CH₄ IRMS system consists of a 1/8" SS tube of which the central 6 cm are packed with Hayesep D (mesh 80/100, Alltech GmbH, Germany). At –132 °C, the PRECON adsorbs CH₄ while O₂ and N₂ are purged out to the vent. After 540 s of preconcentration, the cooling is stopped, the PRECON system slowly warms up, and residual air is vented. Only shortly before the CH₄ is released from the PRECON (at a temperature reading of ~ –75 °C), V1 switches to “inject”. The CH₄ released is thus transferred to the CRY-OFOCUS unit (Fig. 1), while other condensable gases are still retained on the Hayesep

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



D. The CRYOFOCUS unit is a 1/16" gas chromatography (GC) column (Poraplot Q) cooled to -158°C where CH_4 is focussed to obtain a narrow peak and remaining interferences are separated and removed (Brass and Röckmann, 2010). Following the CRYOFOCUS, CH_4 is transferred through V2 to the conversion oven.

For δD measurements, CH_4 is pyrolysed in an alumina (Al_2O_3) tube (0.8 mm inner diameter (i.d.), Length (L) = 360 mm) at a temperature of $+1300^{\circ}\text{C}$. During pyrolysis, CH_4 is converted to hydrogen (H_2) and carbon (C). C is deposited on the inner surface of the alumina tube, which promotes an efficient pyrolysis and H_2 production (Brass and Röckmann, 2010).

For $\delta^{13}\text{C}$ measurements, CH_4 is combusted to CO_2 in an alumina tube (1 mm i.d., $L = 320$ mm) at $+900^{\circ}\text{C}$. Three Nickel wires (0.25 mm outer diameter (o.d.), Goodfellow, Cambridge Ltd., England) are used as catalysts and introduced into the tube. During each run, the combustion tube is flushed with O_2 for 5 s to refresh the oxidant before CH_4 reaches the reactor.

The simultaneous analysis of both δD and $\delta^{13}\text{C}$ is not possible, thus the system is running either in the pyrolysis or in the combustion mode. Following the pyrolysis/combustion step, the sample is transferred via an open split interface (ThermoFinnigan Gas Bench II, Germany) to the mass spectrometer (ThermoFinnigan Delta plus XL, Germany).

2.1.3 Nitrous oxide IRMS

The N_2O IRMS used is a fully automated system based on (Röckmann et al., 2003b). The sample (N_2O , CO_2 and hydrocarbons) from the extraction system is transferred from T2 to the N_2O PRECON in a He carrier gas flow at 50 ml min^{-1} for 400 s. Ascarite II (~8–20 mesh, Aldrich chemistry, USA) is used to remove >99.999 % of the CO_2 and magnesium perchlorate ($\text{Mg}(\text{ClO}_4)_2$) removes the H_2O formed in the reaction of CO_2 with Ascarite. The N_2O is then preconcentrated in a U-shaped SS tube (1.2 mm i.d., $L = 480$ mm) at -196°C , while the residual air is vented. After 400 s, the

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



sample is transferred to the CRYOFCOCUS, which consists of a fused silica capillary (0.53 mm i.d., $L = 460$ mm) cooled to -196 °C. After cryofocusing, the N_2O is purified from remaining CO_2 and hydrocarbons on a GC column (PoraPLOT Q, 0.53 mm i.d., $L = 25$ m) at $+30$ °C and then transferred via a NafionTM dryer to a custom-made open split (Röckmann et al., 2003) and to the mass spectrometer (ThermoFinnigan, Delta Plus XP, Germany). There, the ion masses 44, 45, 46, 30 and 31 are monitored for determination of $\delta^{15}N(N_2O)$, $\delta^{18}O(N_2O)$ and the position dependent ^{15}N signatures ($\delta^{15}N(NO^+ \text{ fragment})$) (Brenninkmeijer and Röckmann, 1999).

2.2 Measurement procedure

2.2.1 Sample preparation and evacuation of the pot

The ice sample is cut with a band saw to the desired size and shape. Subsequently, the sample is microtomed, weighed and inserted into the pre-cooled grating cylinder inside the SS pot. The pot is immediately fixed to the shaking device inside the freezer at -30 °C and connected to the vacuum system via a 65 cm length SS flexible bellows tubing (© Swagelok). Evacuation is usually performed overnight and a vacuum of 10^{-3} mb is reached. The pot containing a new ice sample is evacuated for at least 90 min.

2.2.2 Blank and standard measurement

To diagnose possible contamination and to monitor the stability of the analytical system, a blank and a standard measurement are performed before each ice sample. A blank is also carried out after each sample. In the blank test, we flush pure carrier gas (He) from the extraction system through T2 and T3 (heated to $+60$ °C) to both IRMS systems and verify that neither CH_4 nor N_2O peaks appear in the system. In the standard measurements, about 20-50ml of reference air (NAT332, 2141 ppb CH_4 , 331 ppb N_2O) is filled into the SS pot containing the ice sample for the subsequent run (the pot

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



is evacuated beforehand). The reference air is then extracted like an ice air sample (see next section). The blank and standard measurement ensure that the system is thoroughly evacuated and in a reproducible state before starting with the ice sample.

2.2.3 Ice core air measurement

5 Following the standard measurement, the evacuated SS pot is disconnected from the extraction line and ice grating starts. During the first 2 min the frequency is slowly increased to 1 Hz and then in several steps to 3 Hz (Fig. 2). This is done manually, and by listening, it is taken care that the ice sample does not knock against the walls (lids and bottom) of the SS pot. After 20 min of shaking, the SS pot is reconnected to the
10 glass-line and the transfer line is evacuated. T1 is cooled by an ethanol-liquid nitrogen mixture to -80°C and T2 and T3 are cooled by liquid nitrogen to -196°C . After closing the valve between T1 and T2, the valve of the SS pot is opened and the pressure is measured with a MKS Baratron pressure gauge (range 0–100 mb). This pressure measurement (typically 5–10 mb) is used together with the weight of the ice sample
15 and of both CH_4 and N_2O peak areas to calculate the total amount of air in the ice and the gas mixing ratios. The extraction process starts by opening the valve between T1 and T2. The whole air sample is adsorbed on the Hayesep D in T3 within 45 min; the valve after T3 is kept closed.

After 45 min, the pressure reaches (behind a water trap) 10^{-3} mb and does not decrease further. The valves separating the traps are closed and T2 is heated for 30 s in warm water ($+60^{\circ}\text{C}$) to release the trapped gases (mainly N_2O and CO_2). T3 is placed in a warm water ($+60^{\circ}\text{C}$) bath for at least 20 min to enable complete release of CH_4 . Thereafter, both IRMS systems are started simultaneously and the extracted samples are transferred to the IRMS systems. After isotope measurement of the ice air samples, the glass line is not evacuated, but the second blank measurement as described
25 above is conducted to verify that all the air had been transferred to both IRMS systems.

After the measurement, the SS pot is opened, cleaned with lens paper, filled with new ice, sealed and reconnected to the shaker in the freezer for evacuation.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

⏪

⏩

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



When the two IRMS systems are not analyzing blanks, standards or samples from the ice extraction system, they are automatically running air samples from laboratory reference air cylinders (NAT325 for the CH₄ IRMS and NAT335 for the N₂O IRMS, both filled with atmospheric air cylinders sampled in Groningen, NL) via the separate IRMS systems. Every reference air measurement lasts about 30 min and those runs are used for data correction (see Sect. 3.5) and quality control of the system.

3 Optimization of the dry extraction system

Several parameters were optimized for the new dry extraction system in order to ensure the most precise and reproducible stable isotope measurements.

3.1 Grating efficiency

We optimized the grating efficiency by adjusting the duration, position and frequency of the shaking and the shape of the ice sample in order to have the largest quantity of ice grated in the shortest amount of time. Twenty-two ice core samples (half or quarter cylinders) of 6 to 18cm of length and between 200–800 g weight were introduced into the grater and shaken at frequencies varying from 0 to 3 Hz (Fig. 2). During the shaking tests, the pot was opened every 5min and the remaining (i.e. non-grated) ice samples were weighed to evaluate the grating efficiency. Fig.2 shows the results of the grating tests. It appears that under optimal conditions, (with two half cylinders of 12cm length and at a frequency of 0–3 Hz) 88 % of the ice sample was grated after 10min and 99 % after 20min. The amount of ice introduced into the shaker is not a critical parameter, however, the shaking frequency and the position of the samples in the grater are important. When shaking is started at 3 Hz, a strong knocking against the walls of the SS pot can be heard, which could potentially damage the oxide layer of the SS surface and lead to CH₄ production (Higaki et al., 2006). Furthermore, strong collisions with the wall break the ice sample into small pieces, which decreases the grating efficiency.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

Therefore, the frequency of shaking is increased slowly to 1Hz during the first 2 min, maintained at 1Hz for 4 more min and then increased gradually again to 3 Hz (Fig.2). Moreover, the SS pot can be fixed in the shaking device in different position from the horizontal to the vertical position. For the first 5–10 min of shaking, the pot stays in a horizontal position (angle (a)=0), thereafter it is rotated to an angle (a) of 30°. This allows a more efficient grating of the small remaining pieces. For large samples (>500 g), the grating angle is maintained at $a = 30^\circ$ during the entire grating process to prevent the ice to knock strongly against the lid of the SS pot. The typical diameter of the grated ice flakes is about 1–2 mm and >97 % of the air is extracted while grating bubbly ice.

3.2 Extraction procedure

Extraction of air from the grating pot is a critical step. Since the extraction takes long, it was decided not to pump through a CH₄ adsorption agent with a vacuum pump, but to use a larger quantity of adsorption agent as cryopump. To find the most suitable adsorption agent, several grams of molecular sieve, activated carbon or Hayesep D were filled into separate 100 ml glass bottles, thoroughly outgassed and used to adsorb different amounts of reference air from the SS pot. Hayesep D appears to be the most efficient and reproducible adsorbent. Consequently, in the final design we used a glass-line provided with a 70 ml U-shaped Hayesep D trap (T3).

The N₂O is completely trapped in a U-shaped glass tube (12 mm o.d., $L = 250$ mm) immersed in liquid nitrogen (-196°C), and is released when heated to room temperature. It was verified that no N₂O is trapped in T1 or T3 or remains in T2 after sample transfer to the isotope system by measuring the N₂O mixing ratios from these traps after a normal sample analysis.

3.3 Tests with bubble-free ice

In order to assess potential contamination during the grating-extraction process, nine bubble free (BF) ice samples were analyzed. Those BF ice samples were produced

by introducing Milli-Q water in plastic tubes of 15 cm length and 12 cm of diameter. A slow He flow was then bubbled through the water to purge out air. Subsequently, the plastic tube containing the water was slowly immersed in an ethanol-liquid nitrogen mixture at about -80°C in order to slowly freeze the water from the bottom to the top.

5 Those BF ice samples were then grated in the SS pot containing 20–50 ml of reference air. It should be noted that although this BF ice does not contain air, it is softer than deep ice core ice so that the might not be exactly identical to real ice core sample. After the grating procedure, the reference air from the SS pot was extracted like an ice
10 air sample and CH_4 mixing ratios were measured from T3 on a GC-Flame Ionization Detector (FID, GC8000^{top}, CE instruments). In parallel, the reference air cylinder was analyzed directly on the GC-FID in order to verify that the extracted air had the same mixing ratio as measured directly from the cylinder. The results show no detectable difference, which indicates that no significant contamination occurs during the grating-extraction process.

15 3.4 System reproducibility

More than forty reproducibility tests were conducted by extracting and analyzing between 20 and 100 ml of reference air (NAT332, 2141 ppb CH_4 , atmospheric air cylinder from Groningen) from the SS pot either filled with leftover grated ice samples or empty. NAT332 was regularly measured directly on both IRMS systems as well. The average
20 differences between the isotope signature of NAT332 measured directly on both IRMS systems and extracted from the grating pot shows slight offsets of 0.13‰ for $\delta^{13}\text{C}(\text{CH}_4)$, 0.5‰ for $\delta\text{D}(\text{CH}_4)$, 0.18‰ for $\delta^{15}\text{N}(\text{N}_2\text{O})$, 0.54‰ for $\delta^{18}\text{O}(\text{N}_2\text{O})$, 0.52‰ for $\delta^{15}\text{N}(\text{NO}^+\text{ fragment})$ (Table 1). Those small offsets are constant and daily monitored with the standard measurements. For ice core samples, the reproducibility for different
25 amounts of ice is presented in Table 2. The amount of air remains a limiting parameter for reliable N_2O measurements. Air released from 200 g and 350 g of ice (with mixing ratios of 600–700 ppb for CH_4 and 220–270 ppb for N_2O) is enough for high

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



precision measurements for $\delta^{13}\text{C}(\text{CH}_4)$ and $\delta\text{D}(\text{CH}_4)$, respectively, but for this amount the precision is not very high for the N_2O isotope signatures. An increase of the sample size to about 600 g leads to a strong reduction of the error also for N_2O isotopologues (Table 2).

3.5 Data correction

The isotope analyses are performed on a ThermoFinnigan Delta plus XL IRMS (for CH_4 isotopologues) and on a ThermoFinnigan XP IRMS (for N_2O isotopologues). Running gas peaks of pure CO_2 , H_2 and N_2O bracket the sample peak for direct referencing to eliminate short-term shifts in IRMS performance. This raw δ -value from the chromatogram is evaluated with the ISODAT software and is then compared to the daily mean value of reference air measurements on both IRMS systems to obtain the δ value of the sample versus the reference air, δ_{SAMvsREF} . These values are then corrected for non-linearity when needed (see below). The reference air cylinders have been independently calibrated versus international standards as explained in Brass and Röckmann (2010) and Kaiser et al. (2003).

Linearity tests are performed at least twice a week on both IRMS systems by running twenty-five analyses of various volumes (5 to 40 ml for the CH_4 IRMS and 20 to 333 ml for the N_2O IRMS) of reference air NAT335 (for N_2O IRMS, 326 ppb) and NAT325 (for CH_4 IRMS, 1970ppb) covering the investigated sample range. Those linearity runs are used to monitor the quality of the analytical systems and the stability of the measurements for small peak areas.

The N_2O IRMS system shows non-linearity patterns for $\delta^{15}\text{N}(\text{N}_2\text{O})$ (Fig. 3a) and $\delta^{15}\text{N}(\text{NO}^+ \text{ fragment})$ (Fig. 3c), but not for $\delta^{18}\text{O}(\text{N}_2\text{O})$ (Fig. 3b). To solve this issue, about ten runs with reference air (NAT335) are performed before the ice core air measurement injecting 333ml of NAT335 reference air in order to reach peak areas corresponding to zone C (highest precision zone). The average of those ten runs is defined as δ_{REF_C} . The ice core air sample is related to δ_{REF_C} in order to obtain δ_{SAMvsREF} . In

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

order to correct for the non-linearity, about ten reference air runs are performed covering exactly the same peak area as the ice sample measured beforehand (Fig. 3). The average of those ten runs is $\delta_{\text{REF_lin}}$. The linearity correction (Lin_corr) corresponds to $\delta_{\text{REF_C}} - \delta_{\text{REF_lin}}$. To obtain the final δ value, we add Lin_corr to δ_{SAMvsREF} . Zone A corresponds to $\sim 350\text{--}480$ g of ice samples and zone B to $\sim 500\text{--}700$ g of ice (Table 2). For N_2O isotopologues, the error (standard deviation) decreases by at least 20 % (depending on the isotope) from zone A to zone B. We preferentially measure ice samples in zone B, which is a compromise between good precision and economic use of ice (equivalent to possible high temporal resolution).

The CH_4 IRMS system shows non-linearity patterns (Fig. 4a, b) as well. The correction procedure is similar for N_2O isotopologues, but the number of runs before and after the ice core air run is about six. The amount of ice is less critical for CH_4 isotopologues, because even when measuring ice in zone A, the reproducibility remains good.

4 Intercomparison

No internationally accepted isotope reference materials are currently available for the isotopic composition of CH_4 and N_2O , so different laboratories use different local laboratory reference materials. Therefore, results from different laboratories are generally not directly comparable. Several laboratories are presently involved in isotope measurements of CH_4 and N_2O from the NEEM ice core (North Greenland Eemian Ice Drilling program). As a first step towards characterizing the offset between these laboratories, a small number of air and ice samples were exchanged between Utrecht University and the other laboratories. For CH_4 isotope analysis, air and ice samples were exchanged with the Pennsylvania State University (PSU), the University of Bern (BERN) and the Alfred Wegener Institute for Polar and Marine Research in Bremerhaven (AWI). For N_2O isotope analysis, three air samples were exchanged with the Center for Ice and Climate in Copenhagen (CIC). A larger intercomparison exercise, led by the PSU group, is currently being carried out with many more laboratories.

4.1 Methane intercomparison

Electropolished 2 L stainless steel cans were used for the isotope analysis, similar to those used for air sampling on aircraft and subsequent isotope and trace gas analysis (Kaiser et al., 2006, Laube et al., 2010). For comparison with the PSU lab, three archived firn air samples were used. Two samples (IMAU402 and IMAU724) from the 1999 drilling at Dome C, Antarctica (Bräunlich et al., 2001) and one sample from Svalbard (IMAU490). The fourth sample corresponds to highly enriched CH₄ (IMAU403). For the intercomparison with BERN two continental whole air samples (NAT325 and NAT332) were collected in Groningen, the Netherlands, and used as laboratory reference gases at IMAU. One of them (NAT332) contains a significant CH₄ contamination (mixing ratio 2141 ppb). By combining firn air samples with clean and contaminated recent air samples, the air samples cover a range of ~1.5‰ in $\delta^{13}\text{C}$ and ~35‰ in δD . The very enriched sample (IMAU403) has a ^{13}C content far outside the range of tropospheric values, but it has been included to assess potential differences in the δ scale, which is relevant since most laboratories only use a one-point calibration for CH₄ isotopologues. The ice core samples were from Greenland (B30 core, ~1750 AD), and from Antarctica (B34 core, ~250 AD), provided by AWI and analyzed by BERN, IMAU and AWI, respectively. In addition we used ice from the WAIS divide drilled in 2005 in Antarctica (WDCO5A, ~1550 AD) provided by PSU and analyzed by PSU and IMAU.

Results of the CH₄ intercomparison are summarized in Table 3. For the three firn air samples analyzed by IMAU and PSU (first three lines in Table 3), there is an average offset of $\delta^{13}\text{C}(\text{CH}_4) = 0.28 \pm 0.03\text{‰}$ and $\delta\text{D} = 12.1 \pm 1.5\text{‰}$. This difference is very reproducible, indicating that it is likely due to an offset in calibration scales between the two laboratories. For the WAIS ice core samples (last line in Table 3), the difference is identical for δD (12.4‰), but it increases for $\delta^{13}\text{C}$ to 0.51‰. This effect is larger than the reproducibility established for our new system. It is in the same direction, but slightly larger (~0.1‰) than the difference between air measured directly and extracted from the ice grating device as shown in Table 1. The difference of the IMAU $\delta^{13}\text{C}(\text{CH}_4)$

AMTD

4, 4473–4503, 2011

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



measurements and the results from BERN on ice core air is similar (0.52 ‰), but the difference to AWI is much smaller (0.11 ‰). Unfortunately, no air comparison samples are available for comparison between IMAU, and these two laboratories. For $\delta D(CH_4)$, the results from the IMAU and BERN systems agree very well for both air and ice measurements and the differences are well within the combined error.

The results show that significant scale differences between the individual laboratories exist, which need to be accounted for when comparing data. The difference in offset between IMAU and PSU for air and ice samples indicates that the problem might aggravate when the ice extraction systems is included in the intercomparison. This may be attributed to the difference between the extraction devices used. The IMAU data were obtained with a dry extraction system as described above and the other laboratories use different wet extraction techniques (e.g. Behrens et al., 2008, Bock et al., 2010b, Sowers, 2010).

Concerning the enriched sample (IMAU403), the offset between IMAU and PSU is not consistent with the average offset of the firn air samples. The change in offset is 0.8 ‰ over a range of ~ 20 ‰. The results suggest that future international calibration efforts should aim for at least a two-point calibration strategy for CH_4 isotopologues, where a scale difference can be calibrated like for water isotopologues (SMOW-SLAP-scale). The presented data are only a first step showing the existence of significant differences for $\delta^{13}C(CH_4)$.

The reported differences between different laboratories can be larger than the reported uncertainties of individual laboratories. This means that isotope variations along a polar ice core can be studied consistently and with high precision with one analytical system, but comparisons between datasets should take into account these differences.

An important issue is that possible offsets are constant and do not vary in time, which could be monitored by regularly measuring similar ice core samples. In addition, regular comparisons between wet and dry extraction methods may be used to assess long-term stability of the extraction procedure, and such measurements have been initiated in our laboratory.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

4.2 Nitrous oxide intercomparison

For N₂O, no ice samples have been compared between laboratories yet, but three air cylinders (one with background tropospheric air and two with synthetic air mixtures) have been measured at least five times per cylinder by both IMAU and CIC for $\delta^{15}\text{N}(\text{N}_2\text{O})$ and $\delta^{18}\text{O}(\text{N}_2\text{O})$ (Fig. 5). The gases were selected in order to have a wide isotopic spread. The cylinder with tropospheric background air was sampled at the NEEM deep drilling site in July 2008. For the intercomparison study, the cylinder of NEEM tropospheric background air was used by both laboratories as the reference and isotopes are reported to be consistent with these predicted values. The mean difference between the two laboratories is 0.11 ‰ for $\delta^{15}\text{N}(\text{N}_2\text{O})$ and 0.05 ‰ for $\delta^{18}\text{O}(\text{N}_2\text{O})$, which demonstrates an excellent agreement between IMAU and CIC for air samples. Once the CIC ice system becomes operational, ice core air intercalibration will be performed.

5 Conclusion

A new dry extraction technique coupled to two IRMS systems for simultaneous CH₄ and N₂O isotope analysis has been developed for high-precision isotope measurements of ice core air. The minimum amount of preindustrial ice (with CH₄ mixing ratios of about 600–700 ppb and N₂O mixing ratios of about 220–270 ppb) necessary for measurements of both gases is 350g, but in order to increase reproducibility, we preferentially measure samples of about 600 g. For these amounts, the reproducibility is 2.1 ‰ for $\delta\text{D}(\text{CH}_4)$, 0.18 ‰ for $\delta^{13}\text{C}(\text{CH}_4)$, 0.51 ‰ for $\delta^{15}\text{N}(\text{N}_2\text{O})$, 0.69 ‰ for $\delta^{18}\text{O}(\text{N}_2\text{O})$ and 1.12 for $\delta^{15}\text{N}(\text{NO}^+\text{fragment})$. Possible small offsets during the extraction of air from the grating device are smaller than the presently existing uncertainties of the CH₄ and N₂O isotope scales for all signatures. Results from a small-scale intercalibration exercise for air and ice samples with five external laboratories (BERN, PSU, CIC and AWI) reveal significant offsets between the laboratories. Future attempts for harmonization

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures



Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



of the CH₄ isotope scale should provide at least a two-point calibration scale. Despite these open issues on calibration, the excellent reproducibility will allow the new analytical system to investigate in detail the past atmospheric budget of CH₄ and N₂O with relatively high temporal resolution allowing reconstructing changes in the sources and

5

Acknowledgements. We would like to acknowledge the Dutch NWO for funding (Projects: 851.30.020 & 865.07.001).

References

Behrens, M., Schmitt, J., Richter, K. U., Bock, M., Richter, U. C., Levin, I., and Fischer, H.: A gas chromatography/combustion/isotope ratio mass spectrometry system for high-precision delta $\delta^{13}\text{C}$ measurements of atmospheric CH₄ extracted from ice core samples, *Rapid Commun. Mass Spectrom.*, 22, 3261–3269, doi:10.1002/rcm.3720, 2008.

10

Bernard, S., Röckmann, T., Kaiser, J., Barnola, J.-M., Fischer, H., Blunier, T., and Chappellaz, J.: Constraints on N₂O budget changes since pre-industrial time from new firn air and ice core isotope measurements, *Atm. Chem. Phys.*, 6, 493–503, doi:10.5194/acp-6-493-2006, 2006.

15

Bock, M., Schmitt J., Möller, L., Spahni R., Blunier T., and Fischer H.: Hydrogen isotopes preclude marine hydrate CH₄ emissions at the onset of Dansgaard-Oeschger events, *Science*, 328/5986, 1686–1689, doi:10.1126/science.1187651, 2010a

20

Bock, M., Schmitt, J., Behrens, M., Moller, L., Schneider, R., Sapart, C., and Fischer, H.: A gas chromatography/pyrolysis/isotope ratio mass spectrometry system for high-precision δD measurements of atmospheric CH₄ extracted from ice cores, *Rapid Commun. Mass Spectrom.*, 24, 621–633, doi:10.1002/rcm.4429, 2010b.

25

Bousquet, P., Ciais, P., Miller, J. B., Dlugokencky, E. J., Hauglustaine, D. A., Prigent, C., Van der Werf, G. R., Peylin, P., Brunke, E. G., Carouge, C., Langenfelds, R. L., Lathiere, J., Papa, F., Ramonet, M., Schmidt, M., Steele, L. P., Tyler, S. C., and White, J.: Contribution of anthropogenic and natural sources to atmospheric CH₄ variability, *Nature*, 443, 439–443, doi:10.1038/nature05132, 2006.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Brass, M. and Röckmann, T.: Continuous-flow isotope ratio mass spectrometry method for carbon and hydrogen isotope measurements on atmospheric CH₄, *Atmos. Meas. Tech. Discuss.*, 3, 2433–2476, doi:10.5194/amtd-3-2433-2010, 2010.

Bräunlich, M., Aballain, O., Marik, T., Jockel, P., Brenninkmeijer, C. A. M., Chappellaz, J., Barnola, J. M., Mulvaney, R., and Sturges, W. T.: Changes in the global atmospheric CH₄ budget over the last decades inferred from δ¹³C and δD isotopic analysis of Antarctic firn air, *J. Geophys. Res.*, 106, 20465–20481, doi:10.1029/2001JD900190, 2001.

Brenninkmeijer, C. A. M. and Röckmann, T.: Mass spectrometry of the intramolecular nitrogen isotope distribution of environmental N₂O using fragment-ion analysis, *Rapid Commun. Mass Spectrom.*, 13, 2028–2033, doi:10.1002/(SICI)1097-0231(19991030)13:20<2028::AID-RCM751>3.0.CO;2-J, 1999.

Brenninkmeijer, C. A. M., Janssen, C., Kaiser, J., Röckmann, T., Rhee, T. S., and Assonov, S. S.: Isotope effects in the chemistry of atmospheric trace gases, *Chem. Rev.*, 103, 5125–5162, doi:10.1021/cr020644k, 2003.

Craig, H. and Chou, C. C.: Methane - the Record in Polar Ice Cores, *Geophys. Res. Lett.*, 9, 1221–1224, 1982.

Dlugokencky, E. J., Masarie, K. A., Lang, P. M., and Tans, P. P.: Continuing decline in the growth rate of the atmospheric CH₄ burden, *Nature*, 393, 447–450, doi:10.1038/30934, 1998.

Dlugokencky, E. J., Bruhwiler, L., White, J. W. C., Emmons, L. K., Novelli, P. C., Montzka, S. A., Masarie, K. A., Lang, P. M., Crotwell, A. M., Miller, J. B., and Gatti, L. V.: Observational constraints on recent increases in the atmospheric CH₄ burden, *Geophys. Res. Lett.*, 36, L18803, doi:10.1029/12009gl039780, 2009.

Schmitt, J., Schneider, R., Fischer, H.: A sublimation technique for high-precision measurements of δ¹³CO₂ and mixing ratios of CO₂ and N₂O from air trapped in ice cores, *Atmos. Meas. Tech. Discuss.*, 4, 1853–1892, doi:10.5194/amtd-4-1853-2011, 2011

Etheridge, D. M., Pearman, G. I., and Silva, F. D.: Atmospheric trace-gas variations as revealed by air trapped in an ice core from Law Dome, Antarctica. *Ann. Glaciol.*, 10, 28–33, 1988.

Etheridge, D. M., Steele, L. P., Francey, R. J., and Langenfelds, R. L.: Atmospheric CH₄ between 1000 AD and present: Evidence of antropogenic emissions and climatic variability, *J. Geophys. Res.*, 103, 15979–15993, 1998.

Ferretti, D., Miller, J., White, J., Etheridge, D., Lassey, K., Lowe, D., Allan, B., MacFarling, C., Dreier, M., Trudinger, C., and Ommen, T. v.: Unexpected changes to the global CH₄ budget over the past 2000 years, *Science*, 309, 864–867, doi:10.1126/science.1115193, 2005.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Fischer, H., Behrens, M., Bock, M., Richter, U., Schmitt, J., Loulergue, L., Chappellaz, J., Spahni, R., Blunier, T., Leuenberger, M., and Stocker, T. F.: Changing boreal CH₄ sources and constant biomass burning during the last termination, *Nature*, 452, 864–867, doi:10.1038/nature06825, 2008.

5 Flückiger, J., Monnin, E., Stauffer, B., Schwander, J., Stocker, T. F., Chappellaz, J., Raynaud, D., and Barnola, J. M.: High-resolution Holocene N₂O ice core record and its relationship with CH₄ and CO₂, *Global Biogeochem. Cycles*, 16, 1010, doi:10.1029/2001GB001417, 2002.

Forster, P., Ramaswamy, V., Artaxo, P., Bernsten, T., Betts, R., Fahey, D. W., Haywood, J., Lean, J., Lowe, D. C., Myhre, G., Nganga, J., R. Prinn, Raga, G., Schulz, M., and Dorland, R. v.: Changes in Atmospheric Constituents and in Radiative Forcing, in: *Climate Change 2007: The Physical Science Basis. Contribution of Working Group I to the Fourth Assessment Report of the Intergovernmental Panel on Climate Change* edited by: Solomon, S., Qin, D., Manning, M., Chen, Z., Marquis, M., Averyt, K. B., M. Tignor, and Miller, H. L., Cambridge University Press, Cambridge, United Kingdom and New York, NY, USA, 2007.

15 Güllük, T., Wagner, H. E., and Slemr, F.: A high-frequency modulated tunable diode laser absorption spectrometer for measurements of CO₂, CH₄, N₂O and CO in air samples of few cm³, *Rev. Sci. Instrum.*, 68, 1997.

Güllük, T. and Slemr, F.: Simultaneous measurements of CO₂, CH₄ and N₂O in air extracted by sublimation from Antarctica ice cores: Confirmation of the data obtained using other extraction, *J. Geophys. Res.*, 103, 15971–15978, doi:10.1029/98JD00686, 1998.

20 Higaki, S., Oya, Y., and Makide, Y.: Emission of CH₄ from Stainless Steel Surface Investigate by using Tritium as a Radioactive Tracer, *Chemistry Letters*, 35(3), 292, doi:10.1246/cl.2006.292, 2006.

IPCC: *Climate Change 2007: The Physical Science Basis – Fourth Assessment Report of the Intergovernmental Panel on Climate Change*, Cambridge Univ. Press, New York, 2007.

25 Ishijima, K., Sugawara, S., Kawamura, K., Hashida, G., Morimoto, S., Murayama, S., Aoki, S., and Nakazawa, T.: Temporal variations of the atmospheric N₂O concentration and its delta δ¹⁵N and delta δ¹⁸O for the latter half of the 20th century reconstructed from firn air analyses, *J. Geophys. Res.-Atm.*, 112, D03305, doi:10.1029/2006JD007208, 2007.

30 Kaiser, J., Engel, A., Borchers, R. and Röckmann, T.: Probing stratospheric transport and chemistry with new balloon and aircraft observations of the meridional and vertical N₂O isotope distribution, *Atmos. Chem. Phys.*, 6, 3535–3556, doi:10.5194/acp-6-3535-2006, 2006.

Keppler, F., Hamilton, J. T. G., Brass, M., and Röckmann, T.: CH₄ emissions from terrestrial

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- plants under aerobic conditions, *Nature*, 439, 187–191, doi:10.1038/nature04420, 2006.
- 5 Keppler, F., Hamilton, J. T. G., McRoberts, W. C., Viganò, I., Brass, M., and Röckmann, T.: Methoxyl groups of plant pectin as a precursor of atmospheric CH₄: evidence from deuterium labelling studies, *New Phytol.*, 178, 178, 808–814, doi:10.1111/j.1469-8137.2008.02411.x, 2008.
- Laube, J. C., Martinerie, P., Witrant, E., Brenninkmeijer, C. A. M., Bolder, M., Röckmann, T., van der Veen, C. and Sturges, W. T.: Accelerating growth of HFC-227ea (1,1,1,2,3,3,3-heptafluoropropane) in the atmosphere, *Atmos. Chem. Phys.*, 10, 59903–5910, doi:10.5194/acp-10-5903-2010 2010.
- 10 Lelieveld, J., Crutzen, P. J., and Dentener, F. J.: Changing concentration, lifetimes and climate forcing of atmospheric CH₄, *Tellus*, 50B, 128–150, 1998.
- MacFarling Meure, C., Etheridge, D., Trudinger, C., Steele, P., Langenfelds, R., Ommen, T. v., Smith, A., and Elkins, J.: Law Dome CO₂, CH₄ and N₂O ice core records extended to 2000 years BP *Geophys. Res. Lett.*, 33, L14810, doi:10.1029/12006GL026152, 2006.
- 15 Merritt, D. A., Hayes, J. M., and Des Marais, D. J.: Carbon isotopic analysis of atmospheric CH₄ by isotope-ratio-monitoring gas chromatography-mass spectrometry, *J. Geophys. Res.*, 100 D, 1317/1326, doi:10.1029/94JD02689, 1995.
- Miller, J. B., Mack, K. A., Dissly, R., White, J. W. C., Dlugokencky, E. J., and Tans, P. P.: Development of analytical methods and measurements of δ¹³C in atmospheric CH₄ from the NOAA/CMDL global air sampling network, *J. Geophys. Res.*, 107, 4178, doi:10.1029/2001JD000630, 2002.
- 20 Mischler, J. A., Sowers, T. A., Alley, R. B., Battle, M., McConnell, J. R., Mitchell, L., Popp, T., Sofen, E., and Spencer, M. K.: Carbon and hydrogen isotopic composition of CH₄ over the last 1000 years, *Global Biogeochem. Cycles*, 23, GB4024, doi:10.1029/2009GB003460, 2009.
- 25 Moor, E. and Stauffer, B.: A New Dry Extraction System for Gases in Ice, *J. Glaciol.*, 30, 358–361, 1984.
- Quay, P., Stutsman, J., Wilbur, D., Snover, A., Dlugokencky, E., and Brown, T.: The isotopic composition of atmospheric CH₄, *Global Biogeochem. Cycles*, 13, 445–461, doi:10.1029/1998GB900006, 1999.
- 30 Rice, A. L., Gotoh, A. A., Ajie, H. O., and Tyler, S. C.: High-precision continuous-flow measurement of δ¹³C and δD of atmospheric CH₄, *Anal. Chem.*, 73, 4104–4110, doi:10.1021/ac0155106, 2001.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



- Robbins, R. C., Cavanagh, L. A., and Salas, L. J.: Analysis of Ancient Atmosphere, *J. Geophys. Res.*, 78, 5341–5344, doi:10.1029/JC078i024p05341, 1973.
- Röckmann, T., Kaiser, J., and Brenninkmeijer, C. A. M.: The isotopic fingerprint of the pre-industrial and the anthropogenic N₂O source, *Atmos. Chem. Phys.*, 3, 315–323, doi:10.5194/acp-3-315-2003, 2003a.
- Röckmann, T., Kaiser, J., Brenninkmeijer, C. A. M., and Brand, W. A.: Gas chromatography/isotope-ratio mass spectrometry method for high-precision position-dependent ¹⁵N and ¹⁸O measurements of atmospheric N₂O, *Rapid Commun. Mass Spectrom.*, 17, 1897–1908, doi:10.1002/rcm.1132, 2003b.
- Röckmann, T. and Levin, I.: High-precision determination of the changing isotopic composition of atmospheric N₂O from 1990 to 2002, *J. Geophys. Res.*, 110, D21304, doi:21310.21029/22005JD006066, 2005.
- Schaefer, H., Whiticar, M. J., Brook, E. J., Petrenko, V. V., Ferretti, D., and Severinghaus, J.: Ice Record of δ¹³C for Atmospheric CH₄ Across the Younger Dryas-Preboreal Transition, *Science*, 313, 1109–1112, doi:10.1126/science.1126562, 2006.
- Schäfer, H.: Meteorologische Analyse für Spurengasmessungen am Observatorium Izana (Teneriffa) unter Verwendung von Rückwärtstrajektorien, *Physik, Universität Mainz, Mainz*, 1998.
- Sowers, T.: N₂O record spanning the penultimate deglaciation from the Vostok ice core, *J. Geophys. Res.*, 106, D23, 31903–31914, 2001.
- Sowers, T., Rodebaugh, A., Yoshida, N., and Toyoda, S.: Extending records of the isotopic composition of atmospheric N₂O back to 1800 AD from air trapped in snow at the South Pole and the Greenland Ice Sheet Project II ice core, *Global Biogeochem. Cycles*, 16, 1129, doi:1110.1029/2002GB001911, 2002.
- Sowers, T., Alley, R. B., and Jubenville, J.: Ice core records of atmospheric N₂O covering the last 2000 years, *Science*, 301, 945–948, doi:10.1126/science.1085293, 2003.
- Sowers, T., Bernard, S., Aballain, O., Chappellaz, J., Barnola, J. M., and Marik, T.: Records of the δ¹³C of atmospheric CH₄ over the last 2 centuries as recorded in Antarctic snow and ice, *Global Biogeochem. Cycles*, 19, 493–503, doi:2010.1029/2004GB002408, 2005.
- Sowers, T.: Late quaternary atmospheric CH₄ isotope record suggests marine clathrates are stable, *Science*, 311, 838–840, doi:10.1126/science.1121235, 2006.
- Sowers, T.: Atmospheric CH₄ isotope records covering the Holocene period, *Quaternary Sci. Rev.*, 29, doi:10.1016/j.quascirev.2009.05.023, 2010.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

[Title Page](#)[Abstract](#)[Introduction](#)[Conclusions](#)[References](#)[Tables](#)[Figures](#)[⏪](#)[⏩](#)[◀](#)[▶](#)[Back](#)[Close](#)[Full Screen / Esc](#)[Printer-friendly Version](#)[Interactive Discussion](#)

- Spahni, R., Chappellaz, J., Stocker, T.F., Loulergue, L., Hausammann, G., Kawamura, K., Flückiger, J., Schwander, J., Raynaud, D., Masson-Delmotte, V., Jouzel, J.: Atmospheric methane and nitrous oxide of the late Pleistocene from Antarctic ice cores, *Science*, 310, 1317, doi:10.1126/science.1120132, 2005.
- 5 Vigano, I., van Weelden, H., Holzinger, R., Keppler, F., McLeod, A., and Röckmann, T.: Effect of UV radiation and temperature on the emission of CH₄ from plant biomass and structural components, *Biogeosciences*, 5, 937–947, doi:10.5194/bg-5-937-2008, 2008.
- Vigano, I., Röckmann, T., Holzinger, R., van Dijk, A., Keppler, F., Greule, M., Brand, W. A., Geilmann, H., and van Weelden, H.: The stable isotope signature of CH₄
10 emitted from plant material under UV irradiation, *Atmos. Environ.*, 43, 5637–5646, doi:5610.1016/j.atmosenv.2009.5607.5046, 2009.
- Vigano, I., Holzinger, R., Keppler, F., Greule, M., Brand, W. A., Geilmann, H., van Weelden, H., and Röckmann, T.: Water drives the deuterium content of the CH₄ emitted from plants, *Geochim. Cosmochim. Act.*, 74, 3865–3873, doi:10.1016/j.gca.2010.03.030, 2010.
- 15 Werner, R. A. and Brand, W.A.: Referencing strategies and techniques in stable isotope ratio analysis, *Rapid Commun. Mass Spectrom.*, 15, 501–519, doi:10.1002/rcm.258, 2001.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Table 2. System reproducibility. Five samples of similar ice were measured for each test. For each isotope signature, the first line gives the reproducibility for the minimum amount of ice necessary for reliable measurements and the second line gives the reproducibility for our preferred conditions, which is a trade-off between high precision and possible high temporal resolution.

Stable isotope	Gas amount (ng)	Ice amount (g) 600–700 ppb for CH ₄ 220–270 ppb for N ₂ O	1 σ -reproducibility (‰)
$\delta^{13}\text{C}(\text{CH}_4)$	~ 14	~ 200	0.31
	~ 42	~ 600	0.18
$\delta\text{D}(\text{CH}_4)$	~ 21	~ 350	2.9
	~ 42	~ 600	2.1
$\delta^{15}\text{N}(\text{N}_2\text{O})$	< 10	~ 350	0.92
	> 17	~ 600	0.51
$\delta^{18}\text{O}(\text{N}_2\text{O})$	< 10	~ 350	1.08
	> 17	~ 600	0.69
$\delta^{15}\text{N}(\text{NO}^+\text{fragment})$	< 10	~ 350	1.63
	> 17	~ 600	1.12

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Table 3. Intercomparison of measurements made at IMAU with the new system and at other labs for air samples (six first lines) and ice samples (three last lines) .1 sigma standard deviations from N-measurements are presented between brackets. All data are referenced to V-SMOW for $\delta D(CH_4)$ and V-PDB for $\delta^{13}C(CH_4)$.

Sample type	Sample ID (CH ₄ mix. ratio)	N	$\delta^{13}C(CH_4)$ (‰)		$\delta^{13}C_{\text{IMAU}} - \delta^{13}C_{\text{ex.lab}}$ Ext. Lab	$\delta D(CH_4)$ (‰)		$\delta D_{\text{IMAU}} - \delta D_{\text{ex.lab}}$ Ext. lab
			IMAU	Ext. lab		IMAU	Ext. lab	
Firn air (Dome C)	IMAU724 (1604 ppb)	> 6	-48.66 (0.18)	-48.96 (0.21)	0.30‰ PSU	-75.8 (0.4)	-89.6 (2.5)	13.8‰ PSU
Firn air Dome C	IMAU402 (1701 ppb)	> 6	-47.49 (0.12)	-47.78 (0.13)	0.29‰ PSU	-67.8 (1.9)	-78.9 (1.3)	11.1‰ PSU
Firn air Svalbard	IMAU490 (1821ppb)	> 6	-47.32 (0.14)	-47.57 (0.11)	0.25‰ PSU	-83.9 (0.8)	-95.3 (1.7)	11.4‰ PSU
Ambient air	NAT325 (1970 ppb)	> 50	-47.24 (0.18)	/	/	-88.3 (2.2)	-89.4 (1.7)	1.1‰ BERN
Ambient air	NAT332 (2141 ppb)	> 50	-48.68 (0.08)	/	/	-107.4 (2.3)	-106.3 (1.2)	-1.1‰ BERN
Enriched air	IMAU403 (1906ppb)	> 6	-28.60 (0.02)	-28.11 (0.07)	-0.49‰ PSU	+23.5 (0.4)	+15.1 (0.4)	8.4‰ PSU
Ice Greenland	B30 (~1750 AD)	> 6	-48.44 (0.27)	-48.96 (0.16)	0.52‰ BERN	-94.9 (2.8)	-94.7 (3.7)	0.2‰ BERN
Ice Antarctica	B34 (~250 AD)	> 5	-46.46 (0.21)	-46.57 (0.13)	0.11‰ AWI	-80.5 (3.1)	/	/
Ice Antarctica	WDC05A (~1550 AD)	6(¹³ C) 2(D)	-47.10 (0.08)	-47.61 (0.30)	0.51‰ PSU	-75.9 (2.8)	-88.3 (4.0)	12.4‰ PSU

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

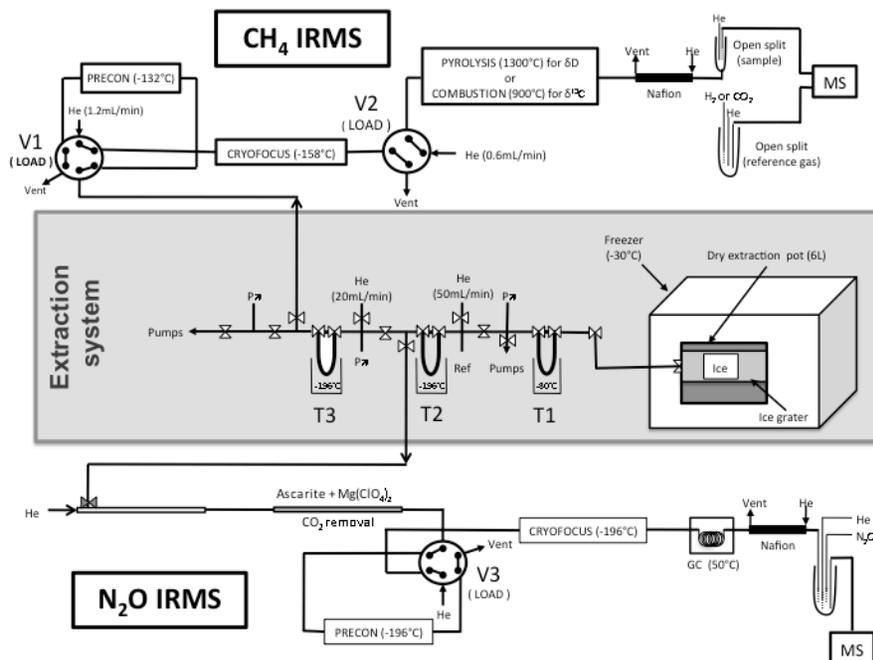


Fig. 1. Schematic set-up of the analytical system. The extraction system in the shaded box in the center consists of a glass line (12 mm o.d.) with manual valves. The connection between this glass line and the ice grater is made via a piece of flexible stainless steel bellows tubing. T1, T2 and T3 represent, respectively, a water trap, a CO₂/N₂O trap and a Hayesep trap where CH₄ and air are adsorbed. V1, V2 and V3 represent multiport two-position Valco valves.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

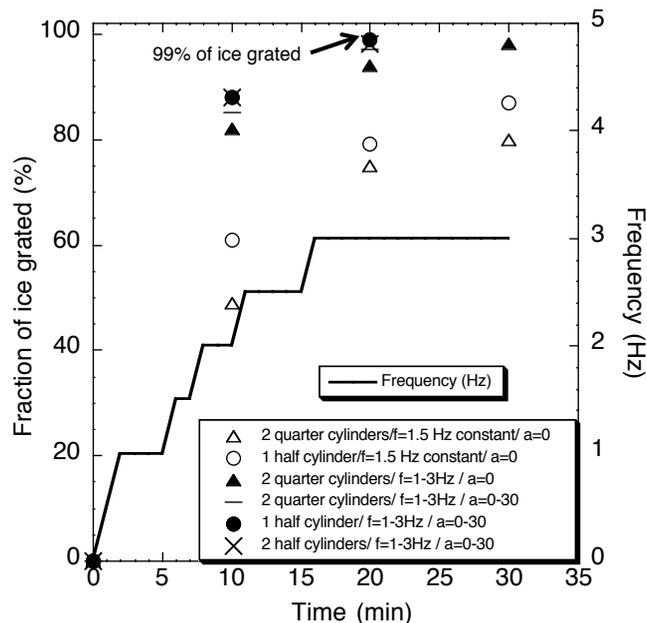


Fig. 2. Grating of twenty-two ice core samples of different length and different shapes at various frequencies and shaking angles (**a**). “a” is the angle between the horizontal plane and the cross section of the SS pot. The error estimate (smaller than the data-points) includes the error of the scale and the spread from repeated tests.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion



Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

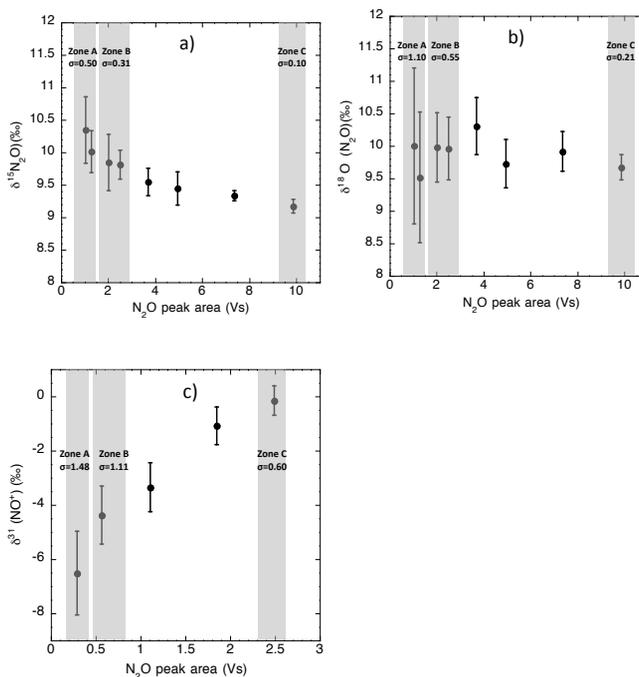


Fig. 3. Results from linearity tests for N_2O isotopologues carried out twice a week during one month. Various amounts of reference air were introduced directly to the N_2O IRMS system. Zone A corresponds to peak areas where the small ice core samples of B30 were measured (350–480 g). Zone B corresponds to the “optimal zone” where larger ice samples (~500–700g) are measured. Zone C corresponds to standard reference air measurements. **(a)** $\delta^{15}N(N_2O)$ **(b)** $\delta^{18}O(N_2O)$ **(c)** $\delta^{15}N(NO^+ \text{ fragment})$.

[Title Page](#)
[Abstract](#)
[Introduction](#)
[Conclusions](#)
[References](#)
[Tables](#)
[Figures](#)
[◀](#)
[▶](#)
[◀](#)
[▶](#)
[Back](#)
[Close](#)
[Full Screen / Esc](#)
[Printer-friendly Version](#)
[Interactive Discussion](#)


Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

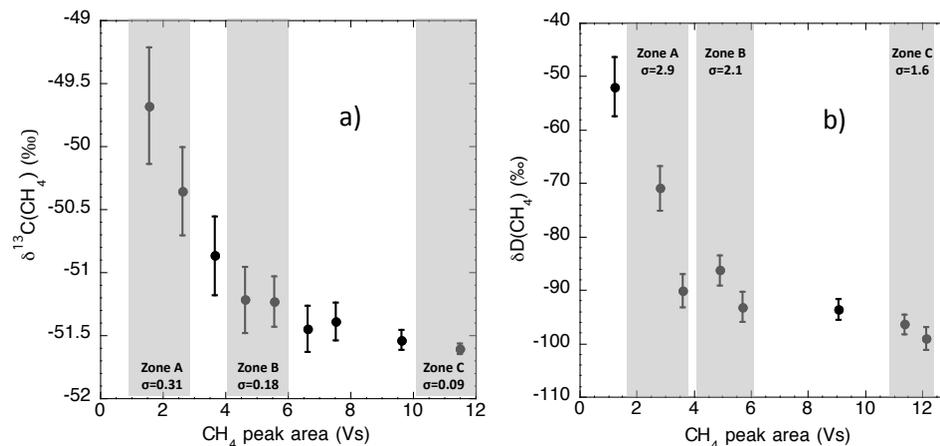


Fig. 4. Results from linearity tests for CH₄ isotopologues carried out twice a week during one month. Various amounts of reference air were introduced directly to the CH₄ IRMS system. Zone A corresponds to peak areas where the small ice core samples of B30 were measured (200–350 g for $\delta^{13}\text{C}$ and 350–480 g for δD). Zone B corresponds to the “optimal zone” where larger ice samples (~500–700 g) are measured. Zone C corresponds to standard reference air measurements. **(a)** $\delta^{13}\text{C}(\text{CH}_4)$ **(b)** $\delta\text{D}(\text{CH}_4)$.

Simultaneous stable isotope analysis of methane

C. J. Sapart et al.

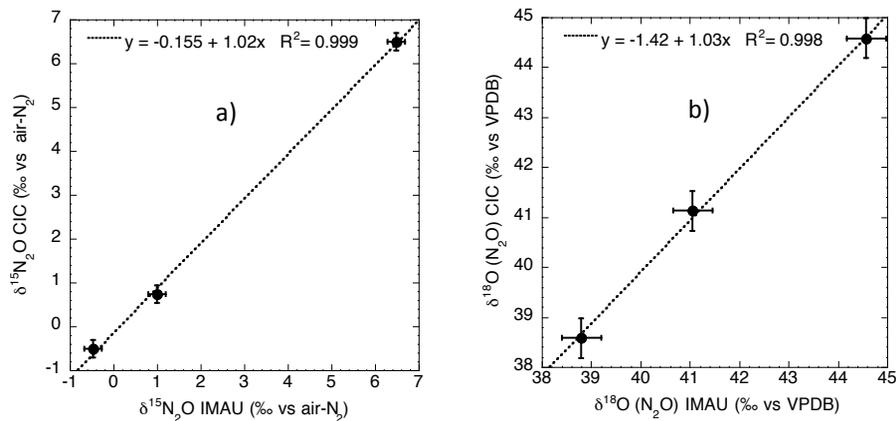


Fig. 5. N_2O isotope results of three air cylinders measured at IMAU and CIC. **(a)** $\delta^{15}\text{N}$ **(b)** $\delta^{18}\text{O}$.

Title Page

Abstract

Introduction

Conclusions

References

Tables

Figures

◀

▶

◀

▶

Back

Close

Full Screen / Esc

Printer-friendly Version

Interactive Discussion

